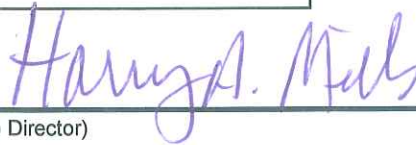


# MicroMacro

Analytical Laboratories

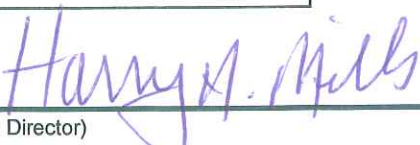
Micro-Macro International, Inc  
183 Paradise Blvd. Suite 108, Athens GA 30607 USA  
Telephone 706 / 548 4557 Fax 706 / 548 4891

<b>Acquisition Date</b>	5/28/2009
<b>Sample Number</b>	Blank
<b>Sample Description</b>	Water Blank
<b>As mg/Kg</b>	0.007
<b>As 3050/6010A</b>	MDL: 0.100
<b>Cd mg/Kg</b>	0.000
<b>Cd 3050/6010A</b>	MDL: 0.100
<b>Cr mg/Kg</b>	0.000
<b>Cr 3050/6010A</b>	MDL: 0.100
<b>Co mg/Kg</b>	0.000
<b>Co 3050/6010A</b>	MDL: 0.050
<b>Cu mg/Kg</b>	0.009
<b>Cu 3050/6010A</b>	MDL: 0.050
<b>Pb mg/Kg</b>	0.168
<b>Pb 3050/6010A</b>	MDL: 0.100
<b>Mo mg/Kg</b>	0.005
<b>Mo 3050/6010A</b>	MDL: 0.100
<b>Ni mg/Kg</b>	0.000
<b>Ni 3050/6010A</b>	MDL: 0.100
<b>Se mg/Kg</b>	0.000
<b>Se 3050/6010A</b>	MDL: 0.050
<b>Zn mg/Kg</b>	0.002
<b>Zn 3050/6010A</b>	MDL: 0.050
<b>Hg mg/kg</b>	0.000
<b>Hg 7471 A</b>	MDL: 0.050 ppm

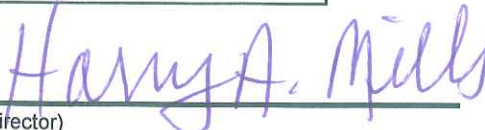


(Lab Director)

<b>Acquisition Date</b>	5/28/2009
<b>Sample Number</b>	MQC
<b>Sample Description</b>	10 ppm Quality Control Standard
<b>As mg/Kg</b>	10.28
<b>As 3050/6010A</b>	MDL: 0.100
<b>Cd mg/Kg</b>	10.51
<b>Cd 3050/6010A</b>	MDL: 0.100
<b>Cr mg/Kg</b>	10.17
<b>Cr 3050/6010A</b>	MDL: 0.100
<b>Co mg/Kg</b>	10.28
<b>Co 3050/6010A</b>	MDL: 0.050
<b>Cu mg/Kg</b>	9.98
<b>Cu 3050/6010A</b>	MDL: 0.050
<b>Pb mg/Kg</b>	9.98
<b>Pb 3050/6010A</b>	MDL: 0.100
<b>Mo mg/Kg</b>	10.34
<b>Mo 3050/6010A</b>	MDL: 0.100
<b>Ni mg/Kg</b>	10.07
<b>Ni 3050/6010A</b>	MDL: 0.100
<b>Se mg/Kg</b>	10.21
<b>Se 3050/6010A</b>	MDL: 0.050
<b>Zn mg/Kg</b>	10.30
<b>Zn 3050/6010A</b>	MDL: 0.050
<b>Hg mg/kg</b>	0.2 ppm QC read 0.200
<b>Hg 7471 A</b>	MDL: 0.050 ppm

  
\_\_\_\_\_  
(Lab Director)

<b>Acquisition Date</b>	5/28/2009
<b>Sample Number</b>	090997-1 Spike
<b>Sample Description</b>	Surround WP
<b>As mg/Kg</b>	99.23%
<b>As 3050/6010A</b>	MDL: 0.100
<b>Cd mg/Kg</b>	103.44%
<b>Cd 3050/6010A</b>	MDL: 0.100
<b>Cr mg/Kg</b>	99.82%
<b>Cr 3050/6010A</b>	MDL: 0.100
<b>Co mg/Kg</b>	102.40%
<b>Co 3050/6010A</b>	MDL: 0.050
<b>Cu mg/Kg</b>	106.64%
<b>Cu 3050/6010A</b>	MDL: 0.050
<b>Mo mg/Kg</b>	99.68%
<b>Mo 3050/6010A</b>	MDL: 0.100
<b>Ni mg/Kg</b>	97.72%
<b>Ni 3050/6010A</b>	MDL: 0.100
<b>Pb mg/Kg</b>	73.50%
<b>Pb 3050/6010A</b>	MDL: 0.100
<b>Se mg/Kg</b>	90.75%
<b>Se 3050/6010A</b>	MDL: 0.050
<b>Zn mg/Kg</b>	104.32%
<b>Zn 3050/6010A</b>	MDL: 0.050
<b>Hg mg/kg</b>	84.40%
<b>Hg 7471 A</b>	MDL: 0.200

  
(Lab Director)

<b>Acquisition Date</b>	5/28/2009
<b>Sample Number</b>	090997-1
<b>Sample Description</b>	Surround WP
<b>As mg/Kg</b>	4.754
<b>As 3050/6010A</b>	MDL: 0.100
<b>Cd mg/Kg</b>	0.000
<b>Cd 3050/6010A</b>	MDL: 0.100
<b>Cr mg/Kg</b>	1.635
<b>Cr 3050/6010A</b>	MDL: 0.100
<b>Co mg/Kg</b>	0.316
<b>Co 3050/6010A</b>	MDL: 0.050
<b>Cu mg/Kg</b>	1.289
<b>Cu 3050/6010A</b>	MDL: 0.050
<b>Mo mg/Kg</b>	1.395
<b>Mo 3050/6010A</b>	MDL: 0.100
<b>Ni mg/Kg</b>	0.743
<b>Ni 3050/6010A</b>	MDL: 0.100
<b>Pb mg/Kg</b>	0.000
<b>Pb 3050/6010A</b>	MDL: 0.100
<b>Se mg/Kg</b>	2.452
<b>Se 3050/6010A</b>	MDL: 0.050
<b>Zn mg/Kg</b>	0.557
<b>Zn 3050/6010A</b>	MDL: 0.050
<b>Hg mg/kg</b>	0.000
<b>Hg 7471 A</b>	MDL: 0.200

  
(Lab Director)